

PCT

WORLD INTELLECTUAL PROPE  
International Bu

INTERNATIONAL APPLICATION PUBLISHED UNDER



(51) International Patent Classification<sup>5</sup> :  
A61B 5/05

A1

(11) Int

WO 9608199A1

(43) International Publication Date: 21 March 1996 (21.03.96)

(21) International Application Number: PCT/US94/10533

(22) International Filing Date: 16 September 1994 (16.09.94)

(71) Applicant: FISCHER IMAGING CORPORATION [US/US];  
12300 North Grant Street, Denver, CO 80241 (US).

(72) Inventor: SICZEK, Bernard; 1252 Chinook Way, Boulder, CO  
80303 (US).


(74) Agents: FISCHMANN, Kent, A. et al.; Sheridan Ross &  
McIntosh, 35th floor, 1700 Lincoln Street, Denver, CO  
80203 (US).

(81) Designated States: JP, European patent (AT, BE, CH, DE, DK,  
ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).

Published

With international search report.

(54) Title: MAGNETIC RESONANCE IMAGING DEVICE FOR TOOL GUIDING

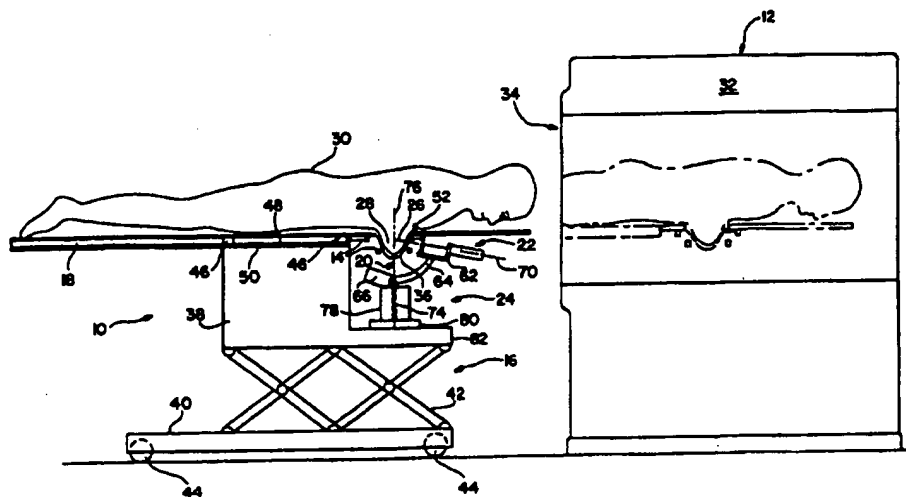

(57) Abstract

The disclosed system (10) employs an MRI device to identify the location of an area of interest within a patient's breast (28) and guide a medical instrument (26) for insertion to the identified location. The patient (30) is positioned on a table top (18) having an opening (52) through which the patient's breast (28) pendulantly projects. The pendant breast (28) is immobilized by a basket (36). The table top (18) and patient (30) are then introduced into magnetic field generator (12) and MRI signals are received by receiver (14). The location of an area of interest within the patient's breast (28) is determined based on the received signals. A guidance assembly (24) can then be used to aim the medical instrument (26) towards the location of interest via a penetration path selected so as to avoid the receiver (14) and basket (36).

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

## MAGNETIC RESONANCE IMAGING DEVICE FOR TOOL GUIDING

## FIELD OF THE INVENTION

5        This invention relates generally to breast imaging and, in particular, to a device which employs magnetic resonance imaging for locating an area of interest within a patient's breast and which is also useful for guiding a medical instrument to the area of interest. The device is  
10 particularly useful for sampling, excising or treating breast lesions including lesions suspected of being cancerous.

## BACKGROUND OF THE INVENTION

15        X-ray mammography has long been considered the "gold standard" of breast imaging and is well-developed and capable of yielding outstanding image resolution. In x-ray mammography, x-rays are transmitted through the patient's breast and impinge upon x-ray film or a digital imaging  
20 camera. Internal features of the patient's breast are depicted as shadows in the resulting image due to differences in x-ray absorption between differing types of tissue. Ordinarily, the patient's breast is compressed during x-ray mammography so that the breast is of more  
25 uniform thickness, thereby enhancing the resulting image. In addition to pure imaging applications such as patient screening or diagnosis, x-ray mammography has been used to localize breast lesions for needle biopsy or for placement

-2-

of a wire or markings to guide a surgeon during subsequent surgical biopsy.

Recently, magnetic resonance imaging (MRI) has been investigated for use in breast imaging. Generally, in MRI, atomic nuclei which possess nuclear magnetic momentum, or spin, are first aligned in a relatively strong magnetic field and are then excited by radio frequency (RF) resonance energy. When their spin returns to equilibrium they emit energy in the form of an RF signal. The time of emission of the absorbed energy, called the relaxation time, depends on magnetic properties of the tissue. The emitted signal can be analyzed to obtain imaging information regarding the tissue under examination. Ordinarily, specified regions or slices of the tissue are sequentially examined so that a composite image of the tissue under examination is obtained.

MRI is of interest to breast imaging specialists for various reasons. Initially, MRI avoids cumulative radiation exposure, a concern expressed by some in connection with alternative x-ray imaging techniques. Additionally, MRI reduces the need to compress the patient's breast to a uniform thickness, thereby potentially enhancing patient comfort. Moreover, MRI may provide imaging advantages for certain soft tissue imaging applications due to its reliance on nuclear magnetic relaxation times rather than x-ray absorption or other characteristics. Advances in MRI technology are also improving MRI resolution.

-3-

However, as to breast imaging, a number of challenges remain in realizing the full potential of MRI. For example, conventional tunnel MRI devices where a patient is axially positioned within a magnetic tunnel are intended for obtaining a composite image from axial body slices. These systems are not tailored for breast imaging and, standing alone, are not capable of yielding the images necessary for increasingly acute breast diagnostic techniques.

Moreover, known MRI devices are not adapted for use in localizing a breast lesion so as to permit insertion of a medical instrument to sample, excise or treat the lesion. With regard to conventional tunnel MRI devices, due to space limitations within the tunnel bore, it is impractical to perform procedures involving insertion of a medical instrument into a patient's breast while the patient remains in an imaging position within the bore. In addition, such devices do not provide a mechanism for allowing localization of a breast lesion after the patient has been withdrawn from the tunnel bore. Known MRI devices which are dedicated to breast imaging generally include magnetic generators and signal transmitters/receivers which surround the patient's breast. These components can interfere with conventional medical instrument insertion devices.

25

#### SUMMARY OF THE INVENTION

The present invention provides an MRI device generally useful for imaging a patient's breast, and particularly apt

-4-

for localizing an area of interest within the patient's breast and readily and accurately obtaining a sample therefrom by insertion of a medical instrument. The invention can advantageously utilize elements of a conventional tunnel MRI device, as is often available on premises, thereby simplifying device construction. Additionally, the device provides for breast specific MRI without interfering with medical device insertion.

According to one aspect of the invention, an MRI/guidance device includes a breast imaging assembly comprising an MRI signal receiver, such as a coil for receiving radio frequency signals, which is dimensioned to receive the breast under examination. The receiver coil can also be utilized, in cooperation with a magnetic field generator for producing a local magnetic field, to transmit an MRI signal.

Alternatively, the transmitted MRI signal, or just the magnetic field employed in transmitting the signal, can be provided by a conventional tunnel MRI device. In one embodiment, a specialized table is provided for supporting the patient and a signal receiver and for permitting the patient and receiver to be introduced into the bore of a conventional tunnel MRI device. The table supports the patient in a prone position and includes an opening through which the patient's breast is permitted to pendulantly protrude. The receiver is supported by the table such that the receiver surrounds the patient's pendant breast. In this manner, elements of a conventional tunnel MRI device

-5-

can be utilized while obtaining the advantages of a localized receiver. The table is moveable between an extended position where the patient's breast is centrally disposed within the bore of the MRI tunnel and a retracted position where the patient is withdrawn from the bore. A mechanism such as bumpers, detents or the like is utilized to ensure accurate registration of the table in the extended and retracted positions.

According to another aspect of the invention, the MRI/guidance device includes an assembly for immobilizing the patient's breast such that information obtained via MRI can subsequently be used for identifying an area of interest within the patient's breast and for inserting a medical instrument to the identified area of interest. The patient's breast is immobilized by a contractible basket which engages the patient's breast. The basket is disposed between the signal receiver and the patient's breast. Preferably, the basket is shaped to generally conform to the contours of the patient's breast and includes a number of openings to allow for insertion of a medical instrument therethrough. In one embodiment, the basket is formed in two halves which are interconnected using a spring or other resilient member so that the halves are drawn towards a contracted position to engage the patient's breast.

According to a further aspect of the present invention, the MRI/guidance device includes a medical instrument guidance assembly for aiming a medical instrument to an identified area of interest within the

-6-

patient's breast. Based on MRI information, the guidance assembly directs a medical instrument towards the area of interest via a penetration path which avoids obstructions such as the signal receiver and/or breast immobilization  
5 assembly.

In this regard, the guidance assembly supports the medical instrument so that the medical instrument is moveable between at least a first position and a second position wherein the medical instrument is aimed at a  
10 common point, the isocenter, in each of the first and second positions. For example, the medical instrument can be orbitally moved relative to the isocenter so that the medical instrument pivots thereabout in a single plane (defined by movement of the aiming axis) and/or the medical  
15 instrument can be rotationally moved relative to the isocenter so that the puncture instrument pivots thereabout in three-dimensions. Aiming the medical device at the area of interest is accomplished by moving the patient and/or guidance assembly so that the area of interest coincides  
20 with the isocenter. The medical instrument can then be inserted to the area of interest for sampling, excision or treatment as desired.

The present invention thus allows for use of a conventional tunnel MRI device while obtaining the  
25 advantages of localized, breast specific signal reception. The invention also allows for insertion of a medical instrument to an identified area of interest within the patient's breast, e.g., a breast lesion, under MRI



-7-

guidance. Further advantages of the present invention will be appreciated upon consideration of the Detailed Description below taken in conjunction with the Drawings.

5

#### BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a side view of a MRI/guidance device constructed in accordance with the present invention;

Fig. 2a is a side view of the medical instrument guidance assembly which forms a portion of the device of  
10 Fig. 1;

Fig. 2b is a cross-sectional view of the medical instrument guidance assembly of Fig. 2a illustrating the slidable interconnection which facilitates orbital movement of the medical instrument;

15 Fig. 3a is a bottom view of the device of Fig. 1 illustrating a technique for positioning the breast immobilization basket and signal receiver coil relative to the patient;

Fig. 3b is a bottom view showing the breast  
20 immobilization basket assembly; and

Fig. 3c is a front view of the breast immobilization basket.

#### DETAILED DESCRIPTION

25 Referring to Figs. 1-3c, an MRI/guidance system is generally identified by the reference numeral 10. The system 10 comprises a magnetic field generator 12, a signal receiver 14, a stretcher assembly 16 including an

-8-

extendible table top 18, a breast immobilization basket assembly 20, a medical instrument insertion assembly 22, and a guidance assembly 24 for aiming a medical instrument 26.

5           The system 10 employs known MRI principles to image a breast 28 of a patient 30. As is known, MRI generally involves subjecting the tissue to be imaged to a strong magnetic field, applying an RF signal to the tissue and receiving an RF signal from the tissue. In accordance with  
10 the present invention, the magnetic field may be specifically directed to the breast under examination via a dedicated magnetic field generator or the less localized magnetic field of a tunnel MRI device may be utilized.

---

          In the illustrated embodiment, the magnetic field  
15 generator 12 comprises a conventional tunnel MRI device as is commonly available at medical imaging facilities, thereby eliminating the need for a magnetic field generator dedicated to breast imaging applications. The generator 12 comprises a resistive or superconductive magnet 32 which is  
20 generally configured in the shape of a cylinder. The illustrated generator can further include a shim coil to correct magnet field inhomogeneities and a gradient coil for producing a magnetic field gradient for encoding spatial information into the imaging signals. In addition,  
25 conventional tunnel MRI systems normally include a body coil for applying an RF signal to the patient 30. As will be described below, this RF signal can alternatively be applied in accordance with the present invention via

-9-

receiver 14. These components are disposed about a central bore 34 of sufficient size to receive the patient 30 therein. The generator 12 may comprise, for example, the SIGMA system manufactured by General Electric.

5         Stretcher assembly 16 is utilized for transporting the patient 30 into and out of bore 34. The stretcher assembly 16 comprises an extendible table top 18 supported by platform 38. Platform 38, in turn, is supported on base 40 via collapsible platform jack 42 so as to allow for  
10         adjustment of the height of table top 18. In this regard, the height of table top 18 is preferably adjusted so that the breast 28 under examination is centrally disposed  
15         within bore 34 for optimal imaging. Conveniently, assembly 16 can be provided with rollers to facilitate positioning of assembly 16 relative to generator 12.

Table top 18 is axially moveable relative to bore 34 between an extended position wherein the patient 30 is disposed within bore 34 for imaging (shown in phantom in Fig. 1) and a retracted position for performing further  
20         medical procedures on the patient's breast 28. To facilitate movement of table top 18, rollers 46 are provided on upper surface 48 of platform 38. The rollers 46 roll in tracks formed in lower surface 50 of table top 18 to ensure that movement of table top 18 is aligned  
25         axially with bore 34. The rollers 46 and the tracks of table top 18 should be formed from non-magnetic materials such as stainless steel to provide for smooth rolling movement of table top 18. It will be appreciated that, in

-10-

the illustrated system 10, all components utilized in close proximity to magnetic generator 12 are formed from materials which do not affect the homogeneity of the magnetic field used. To obtain good images, the magnetic field has to be homogeneous to a very high degree.

As will be understood upon consideration of the description below, it is useful to provide for positive registration of the table top 18 in the extended and retracted positions. In this regard, bumpers can be provided on the upper surface 48 of platform 38 and/or lower surface 50 of table top 18 to positively limit table top movement. Alternatively, a detent may be provided on one of these surfaces or elsewhere to accurately control the relative positioning of table top 18 and platform 38.

As shown, the patient 30 lies in a prone position on table top 18. At least one opening 52 is provided in table top 18 to allow the breast 28 under examination to pendulantly protrude through the table top 18. The illustrated table top includes two openings 52 positioned so that either of the patient's breasts can be examined. This pendant positioning of the patient's breast 28 is advantageous in that the breast 28 is drawn downwardly by gravity, thereby facilitating access to areas of interest within the patient's breast 28 near the chest wall.

The receiver 14 and basket assembly 20 for immobilizing the patient's breast 28 also travel with table top 18 so that a fixed spatial relationship is maintained. As noted above, the receiver 14 is disposed in close

-11-

proximity to the breast 28 under examination and surrounds the breast 28 so as to provide high resolution, breast specific signal reception. In this regard, the illustrated receiver 14 comprises an RF receiver coil provided in a generally conical configuration. The receiver 14, together with the basket assembly 20, as will be described below, is connected to table top 18 so that the receiver surrounds opening 52 in table top 18 to receive the patient's breast 28. In addition, the receiver 14 communicates with a conventional MRI signal processing unit, which can comprise a digital computer, for acquiring data and reconstructing images based on the received signals. The receiver coils can also be utilized to transmit the RF signal which cooperates with the magnetic field to provide the MRI signal.

Basket assembly 20 is interposed between receiver 14 and the patient's breast 28. The basket assembly 20 immobilizes the patient's breast 28 relative to table top 18 so that localization information derived in the MRI procedure can be used in guiding the medical instrument 26 to an area of interest within the patient's breast 28. Accordingly, the basket assembly 20 is connected to table top 18 to receive the breast 28 protruding through opening 52.

As shown most clearly in Figure 3a, the basket assembly 20 comprises a basket 36 formed in two halves which are drawn together to engage the patient's breast 28. The basket 36 is shaped to generally conform to the

-12-

contours of the patient's breast 28 thereby enhancing patient comfort. It will be appreciated that it is unnecessary in MRI to compress the breast 28 to a uniform thickness. In addition, the basket 36 includes a number of openings 54 of any suitable shape to allow insertion of the medical instrument 26 therethrough. Additional baskets 36 of various sizes can be provided for interconnection to table top 18 to accommodate patients of different sizes. The basket 36 is formed from a material such as one of various plastics which does not unduly interfere with the MRI procedure.

The two halves of basket 36 are connected via arms 56 to a common non-magnetic hinge 58 and are drawn together by a non-magnetic spring loaded connection 60. Receiver 14 is also mounted to table top 18 via hinge 58 so as to move with basket 36. The hinge 58 is positioned such that the basket 36 and receiver 14 can be moved across the patient's chest from one breast to the other. In this manner, table top 18 can be utilized to perform medical procedures on either breast without awkwardly positioning the patient 30 on table top 18.

The medical instrument insertion assembly 22 is used to insert a medical instrument 26 to an area of interest within the patient's breast 28 identified through MRI. The nature of the medical instrument 26 and insertion assembly 22 depends on the particular procedure to be performed. One such procedure is a needle biopsy to obtain a cell or tissue sample from a suspicious lesion for diagnosing the

-13-

nature of the lesion, e.g., cancerous, benign, or more specifically, fibroadenoma, ductile carcinoma, etc. Other procedures which can be conducted using the system 10 include various trans-cannula procedures such as  
5 cryoablation, laser ablation, hyperthermia, medicament delivery, percutaneous removal, draining or other procedures for treating or eliminating a lesion, cyst or other area of interest. Thus, the insertion assembly 22 can simply be a guide for facilitating manual insertion of  
10 a biopsy needle, trocar and cannula, or other instrument, or the assembly can be a mechanized delivery system. In the illustrated embodiment, insertion assembly 22 comprises  
a biopsy gun for rapid delivery of a biopsy needle to an identified lesion.

15 The guidance assembly 24 is used for aiming the medical instrument 26 at the identified area of interest within the patient's breast 28 and allows for selection of a penetration path wherein the receiver 14 and basket 36 are avoided. Accordingly, the guidance assembly 24 allows  
20 the medical instrument 26 to pass between the coils of receiver 14 and through an opening 54 of basket 36 en route to the area of interest. The guidance assembly 24 comprises a platform 62 for supporting the medical instrument insertion assembly 22. The platform 62 is mounted on an  
25 arcuate rail 64 which is slidably received within housing 66 via bearings 68 (Fig. 2b). In this manner, the insertion assembly 22 can be orbitally moved by sliding rail 64 within housing 66, as shown in phantom in Fig. 2a, such

-14-

that the aiming axis 70 of medical instrument 26 remains directed at isocenter 72.

In addition, the insertion assembly 22 can be rotationally moved around the patient's breast 28 while the aiming axis 70 of medical instrument 26 remains directed at isocenter 72. Housing 66 is thus mounted on shaft 74 for rotation about shaft axis 76. The intersection of the aiming axis 70 and shaft axis 76 thus defines the isocenter 72. It will thus be appreciated that the combination of orbital and rotational movement of the medical instrument 26 allows for variation of the penetration path of the medical instrument 26 with respect to breast approach angle and with respect to inclination angle relative to the chest wall.

Targeting of an area of interest within the patient's breast is accomplished by positioning the patient 30 and/or the guidance assembly 24 so that the area of interest coincides with the isocenter 72 of guidance assembly 24. In the illustrated embodiment, guidance assembly 24 is moveable relative to stretcher assembly 16 and patient 30. To adjust the height of guidance assembly 24, shaft 74 can be raised or lowered within cylinder 78 mounted on base 80. Base 80 is slidably moveable on recessed surface 78 of platform 38 so that guidance assembly 24 can be moved side-to-side or forward-to-rearward relative to the patient's chest. For example, cylinder 78 can be mounted for forward-to-rearward movement relative to base 80, and base 80 can be mounted for side-to-side movement relative to



-15-

surface 82. Appropriate brakes may be provided between all moveable components of guidance assembly 24 to lock the assembly into a selected position.

In order to allow for accurate targeting of an area of interest within the patient's breast 28, the spatial relationship between the area of interest and guidance assembly 24 must be known. This can be accomplished by providing at least one reference marker which appears in the images used for localizing the area of interest and which has a known location relative to the guidance assembly 24 when the system 10 is configured for medical device insertion. In the illustrated embodiment, this purpose is served by incorporating three high contrast markers into, or attaching three high contrast markers to the basket 36. The markers may comprise oil capsules and/or may include gadolinium or other contrast materials.

Any of the above-described movements of system can be motorized if desired. However, care must be taken to ensure that such motors do not interfere with and are otherwise compatible with the magnetic field generator 12. In this regard, hydraulic motors may be disposed in a separate, shielded room where the necessary power is transmitted to the appropriate components of system 10 by hydraulic lines.

In summary, the system 10 operates as follows. The stretcher assembly is first positioned adjacent the magnetic field generator 12 and the height of the table top 18 is adjusted relative to the bore 34 of generator 12.

-16-

The table top 18 is then extended so that the patient 30 is centrally disposed within bore 34. Receiver 14 is utilized in combination with generator 12 to transmit MRI signals and is also used to receive signals from the tissue under examination. MRI images of the patient's breast 28 are thus obtained. Based on these images, the location of an area of interest within the patient's breast 28 is determined. With the table top 18 in the retracted position, the guidance assembly 24 is positioned so that the isocenter 72 thereof coincides with the identified area of interest. The guidance assembly can then be manipulated to select a penetration path for medical instrument 26 wherein interference with the receiver 24 and basket 36 is avoided.

While various embodiments of the present invention have been described in detail, it is apparent that further modifications and adaptations of the invention will occur to those skilled in the art. However, it is to be expressly understood that such modifications and adaptations are within the spirit and scope of the present invention.

-17-

What is claimed is:

1. An apparatus for use in performing medical procedures on a patient's breast, comprising:

5 immobilizing means for immobilizing said patient's breast;

magnetic resonance imaging means for imaging said patient's breast including transmitting means for applying a signal to said patient's breast and receiving means for receiving a signal from said patient's breast, said  
10 receiving means defining a volume dimensioned for receiving said patient's breast, wherein said magnetic resonance imaging means provides imaging information regarding said patient's breast;

identifying means employing said imaging information  
15 for identifying the location of an area of interest within said patient's breast; and

medical instrument means for inserting a medical instrument to said identified location of said area of interest within said patient's breast.

20 2. The apparatus of Claim 1, wherein said immobilizing means comprises a contractible basket shaped to generally conform to the contours of said patient's breast.

25 3. The apparatus of Claim 1, wherein said immobilizing means comprises a basket formed in two halves which are urged together by a resilient member.

-18-

4. The apparatus of Claim 1, wherein said magnetic resonance imaging means comprises cylindrical magnetic means for receiving said patient therein.

5. The apparatus of Claim 1, further comprising  
5 penetration path selection means for selecting a penetration path for inserting said medical instrument to said identified location of said area of interest within said patient's breast wherein the location of at least one of said immobilizing means and said receiving means is  
10 accounted for in selecting said penetration path.

6. The apparatus of Claim 1, further comprising isocentric support means for movably supporting said medical instrument so that said medical instrument is  
moveable between a first position and a second position  
15 wherein said medical instrument is aimed at an isocenter of said support means in each of said first and second positions.

7. The apparatus of Claim 1, further comprising reference mark means for providing reference marks useful  
20 for establishing a frame of reference for analyzing images of said patient's breast.

8. The apparatus of Claim 7, wherein said reference mark means comprises a contrast material disposed in predetermined spatial location relative to said  
25 immobilization means.

-19-

9. The apparatus of Claim 1, wherein said medical instrument means comprises a biopsy gun for rapid insertion of a biopsy needle to said identified location of said area of interest within said patient's breast.

5 10. The apparatus of Claim 1, further comprising table means for supporting said patient in a prone position, said table means having an opening therein through which said patient's breast is permitted to pendulantly protrude.

10 11. The apparatus of Claim 10, positioning means for moving said table means between a first position wherein said patient's breast is positioned for imaging and a second position wherein said patient's breast is positioned for insertion of said medical instrument.

15 12. An apparatus for use in performing medical procedures on a patient's breast, comprising:

immobilizing means for immobilizing said patient's breast;

20 magnetic resonance imaging means for imaging said patient's breast using a magnetic resonance imaging signal and providing imaging information regarding said patient's breast;

25 identifying means employing said imaging information for identifying the location of an area of interest within said patient's breast;

medical instrument means for inserting a medical instrument to said identified location of said area of interest within said patient's breast; and

-20-

penetration path selection means for selecting a penetration path for inserting said medical instrument means to said identified location of said area of interest within said patient's breast wherein a location of at least  
5 one of said immobilizing means and said magnetic resonance imaging means is accounted for in selecting said penetration path.

13. The apparatus of Claim 12, wherein said penetration path selection means comprises isocentric  
10 support means for movably supporting said medical instrument so that said medical instrument is moveable between a first position and a second position wherein said medical instrument is aimed at an isocenter of said support means in each of said first and second positions.

15 14. The apparatus of Claim 13, wherein said support means is operative for orbitally moving said medical instrument across a range of positions relative to said isocenter, said range of positions defining a substantially planar region.

20 15. The apparatus of Claim 13, wherein said support means is operative for rotationally moving said puncture instrument across a range of positions relative to said isocenter, said range of positions defining a three-dimensional region.

-21-

16. The apparatus of Claim 12, further comprising table means for supporting said patient in a prone position, said table means having an opening therein through which said patient's breast is permitted to  
5 pendulantly protrude.

17. An apparatus for use in performing medical procedures on a patient's breast, comprising:

table means for supporting said patient in a prone position, said table means having an opening therein  
10 through which said patient's breast is permitted to pendulantly protrude;

immobilization means, disposed in predetermined relationship to said table means, for immobilizing said patient's breast in a fixed position with respect to a  
15 predetermined frame of reference;

magnetic resonance imaging means for imaging said patient's breast, said magnetic resonance imaging means including a generally cylindrical component defining an internal axial bore; and

20 positioning means for axially moving said table means relative to said bore between a first position wherein said patient is disposed within said bore for imaging said patient's breast and a second position wherein said patient is disposed outside said bore, wherein said patient's  
25 breast is maintained in said same fixed position with respect to said predetermined frame of reference when said table means is in said first position and when said table means is in said second position.

-22-

18. The apparatus of Claim 17, wherein said immobilizing means comprises a contractible basket shaped to generally conform to the contours of said patient's breast.

5        19. The apparatus of Claim 17, wherein said immobilizing means comprises a basket formed in two halves which are urged together by a resilient member.

20. The apparatus of Claim 17, wherein said immobilizing means is interconnected to said table means so  
10 as to allow for movement of said receiving means across said patient's chest.

21. An apparatus for use in performing medical procedures on a patient's breast, comprising:

table means for supporting said patient in a prone  
15 position, said table means having an opening therein through which said patient's breast is permitted to pendulantly protrude;

transmitting means for transmitting an electromagnetic signal including magnetic means for producing a magnetic  
20 field, said magnetic means including a generally cylindrical component defining an internal axial bore;

receiving means for receiving a signal from said patient's breast, said receiving means defining a volume dimensioned for receiving said patient's pendant breast;  
25 and

positioning means for axially moving said table means relative to said bore between a first position wherein said patient is disposed within said bore for imaging said




-23-


patient's breast and a second position wherein said patient is disposed outside said bore.

22. The apparatus of Claim 22, wherein said receiving means is interconnected to said table means so as to allow  
5 for movement of said receiving means across said patient's chest.

---

FIG. 1

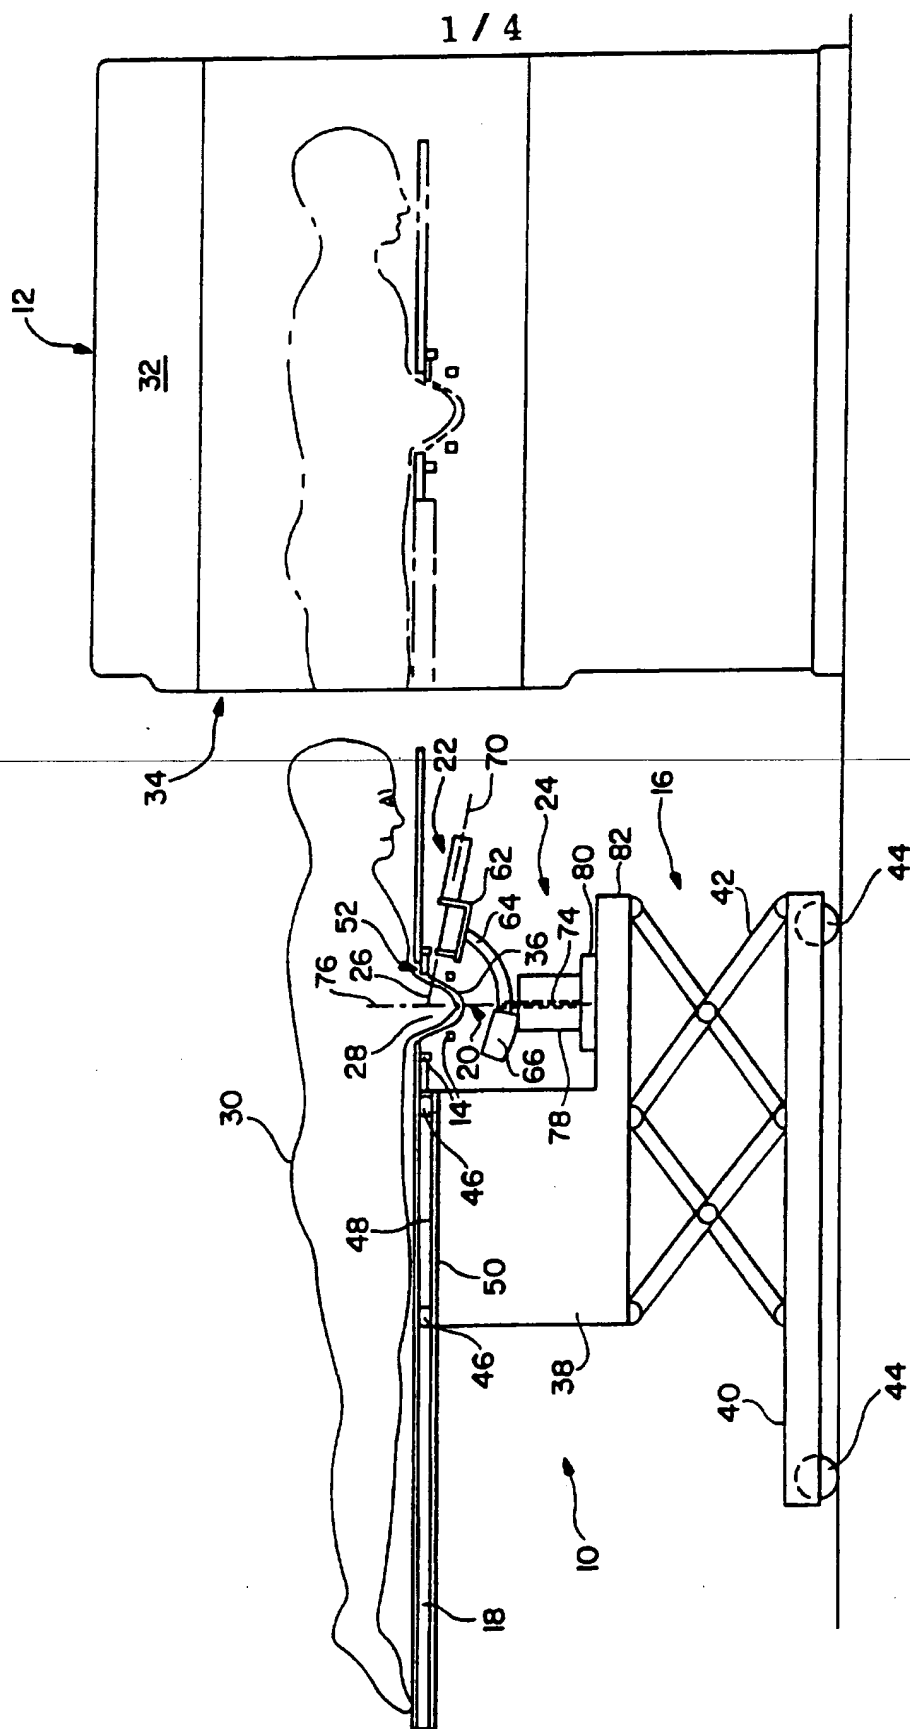

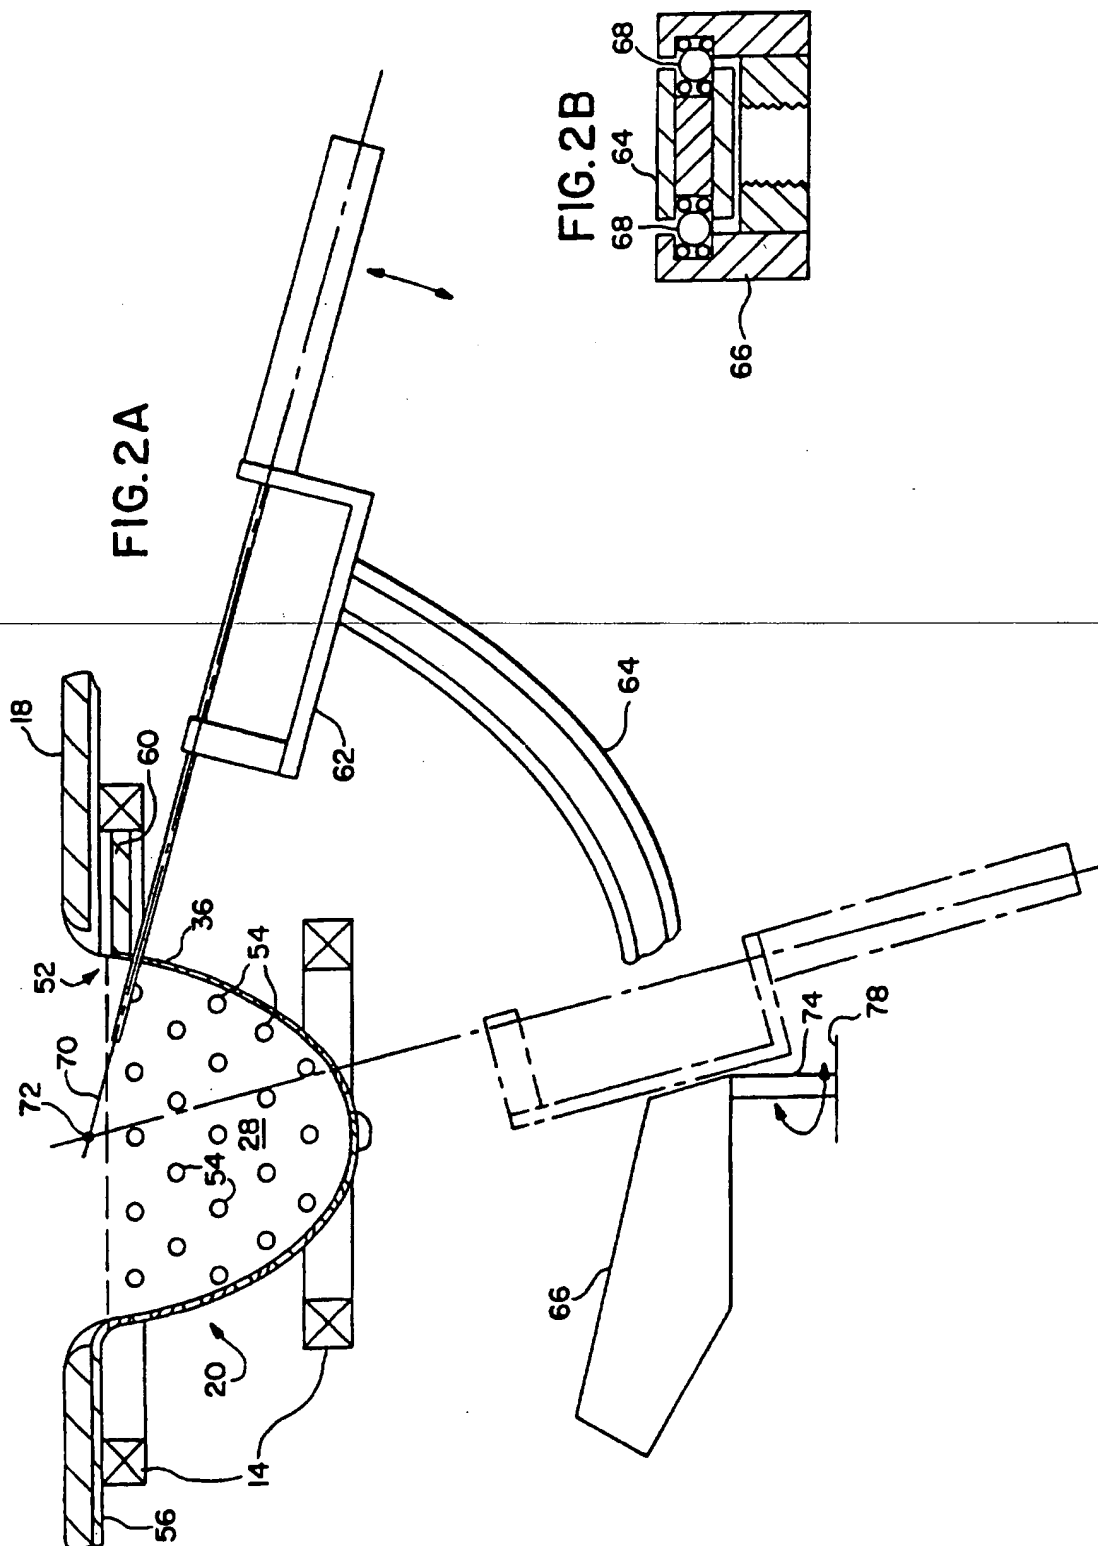

3 / 4

FIG. 3A

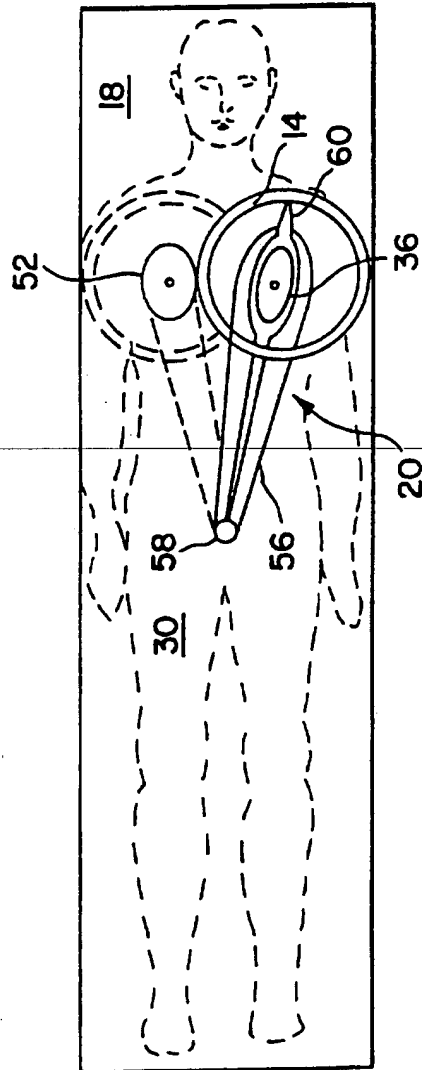


FIG.3B


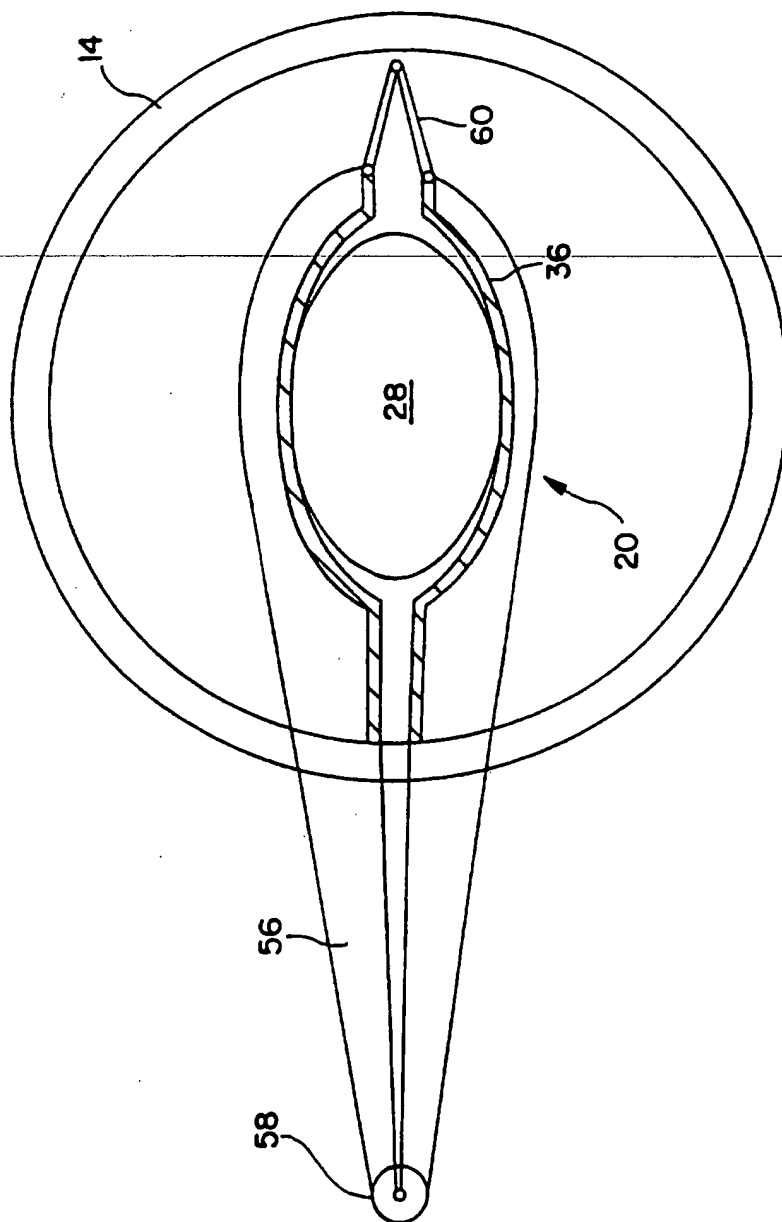


FIG.3C

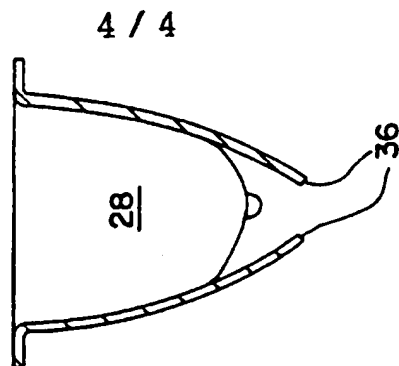

# INTERNATIONAL SEARCH REPORT

International application No.  
PC 1/US94/10533

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(5) :A61B 5/05

US CL :606/130

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 128/653.1; 604/164, 264; 606/130, 185

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

NONE

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

NONE

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US, A, 5,078,142, (SICZEK ET AL.), 07 January 1992. See entire document.	1-22
Y	US, A, 4,608,991, (ROLLWITZ), 02 September 1986. See entire documents.	1-22
Y	US, A, 5,219,351, (TEUBNER ET AL.), 15 June 1993. See entire document.	1-22
Y	US, A, 4,580,561, (WILLIAMSON), 08 April 1986. See entire document.	1-22
Y	US, A, 4,943,986, (BARBARISI), 24 July 1990. See entire document.	1-22

☐ Further documents are listed in the continuation of Box C.

☐ See patent family annex.

* Special categories of cited documents:	T	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
*A* document defining the general state of the art which is not considered to be part of particular relevance	X*	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
*E* earlier document published on or after the international filing date	Y*	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
*L* document which may throw doubt on prior claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	&*	document member of the same patent family
*O* document referring to an oral disclosure, use, exhibition or other means		
*P* document published prior to the international filing date but later than the priority date claimed		

Date of the actual completion of the international search

14 NOVEMBER 1994

Date of mailing of the international search report

DEC 29 1994

Name and mailing address of the ISA/US  
Commissioner of Patents and Trademarks  
Box PCT  
Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer

PETER ASCHENBRENNER

Telephone No. (703) 308-3523